

TBN



Charging DIGI+



Charge fully with Micro-USB cable before first use

Refit USB socket cover



Fully charged battery run time: 50 tests

Note: Charge fully at least once every 6 months

Powering On

Use Left (L), Middle (M) or Right (R) button to power on




Testing - BN - SPOT (single oil test) for DIGI+ BN and DIGI+ Combined



BN compares the pressure generated from a used oil test to a new oil test. For each oil type, new oil is measured and saved as a calibration for future used oil tests.

Calibration

Cell must be calibrated for each of the oil types to be measured using a new sample of unused oil before used oil can be tested.


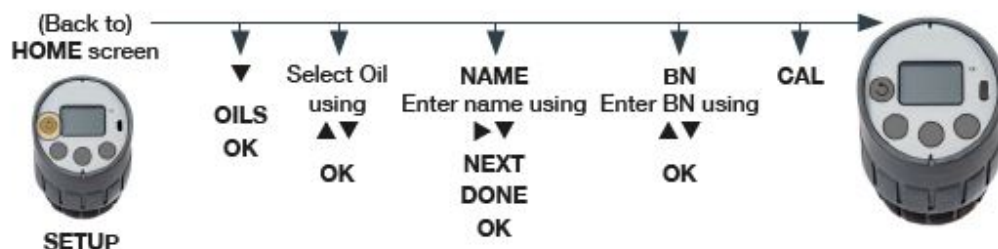


Measure Used Oil

Select Oil using ▲▼ OK → (Follow on-screen instructions)



Note: Close and hand tighten only (1/8 turn max.)



TESTING IS COMPLETE

Check result against limit for the test point

Cleaning



Dispose of contents carefully and wipe with a lint-free cloth. Use a mild solvent if necessary, for example, isopropyl alcohol.

Powering Off



OR

AUTO-OFF after 5 minutes

Test Kits, Spares and Reagents

632406 TBN Reagent Replacement Pack
532430 TBN Reaction Cell



- Quick Start Guide
- Product Data Sheet
- Safety Data Sheet
- Test Cell Utility Software
- Example Utility Files



Adhesive Strip

Adhesive Strip